



# PERFECT MATCH.

# VITA

## VITA MEDIENDATENBANK

### User Manual

<https://mam.vita-zahnfabrik.com>

# Log-in

# VITA



**VITA** Media database

User (E-mail)

Password

Login

[Password forgotten](#)

[Register as new user](#)

 English ▼

Log in with the familiar VITA login credentials:

VITA ID for VITA employees or e-mail address and password.

If you would like to use the media database and are not yet logged in, you can register here.

Changing the language in German, French, Italian or Spanish is possible here.

[Contact & support](#) [Terms of use](#)

# Media search. Symbols

VITA

VITA Media database

Type of media objects

Search

20 of 11526 results




VITA AKZENT Plus CHROMA STAINS

V 005 10375  
DE EN IT ES PL



SD321 VITA AMBRIA

V 005  
DE EN FR IT ES ...

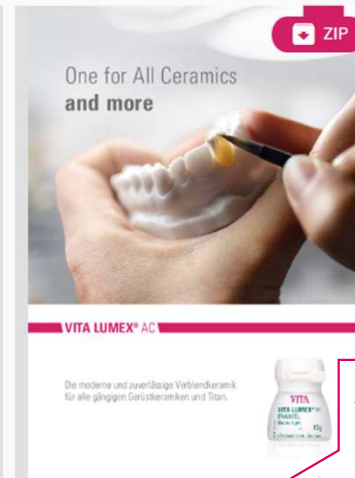

VITA LUMEX AC

V 003 10609  
DE EN FR IT ES ...

Displays the file format.

All brochures are available as a ZIP, as PDFs in several languages are included.

Language icons indicate the languages in which the asset is available.

To download the asset in a specific language, click or double-click. The detailed view opens. See detailed view.

V 003 indicates which version is involved.

10609 indicates the print number.

# Media search. Filter

VITA

**VITA Media database** Contact & support Change password English

Type of media objects  Search

**Filter**

- ☐ Product communication
  - ☐ Offer sheets and sales info
  - ☐ Application pictures
  - ☐ User manuals
  - ☐ Instructions for use
  - ☐ Order blocks
  - ☐ Firing tables
  - ☐ Brochures
  - ☐ CAD drawings
  - ☐ Spare part lists
  - ☐ Press

Search  Reset

20 of 11526 results

**VITAVM.LC**  
Getraufschneidung/Vollversion VITA VM LC und VITA VM LC fibre

**VITA VIONIC SOLUTIONS**

**SD027 VITA VM CC LIQUID**

VITA - perfect match

VITA VIONIC SOLUTIONS

SD027 VITA VM CC LIQUID

V 003 10668M

V 006

This "filter search" can be used to filter according to predefined categories, such as product and publication type (brochure, instructions for use).

The filter selection is started via "Search" and can be cleaned via "Reset".



# Media search. TIP

VITA

The screenshot shows the VITA Media database search interface. At the top, there is a pink header bar with the VITA logo, 'Media database', and links for 'Contact & support', 'Change password', and 'English'. Below the header, a search bar contains the text 'Picture from 10805'. A dropdown menu is open below the search bar, showing suggestions: 'picture', 'pictures', 'from', '10805', and '108050'. A pink information icon (i) is positioned to the left of the dropdown menu. A pink callout box points to the search bar and contains the following text:

**TIP for the image search:**

Search for images using the search term "Picture from" and the print number of the brochure, e.g. 10805: Picture from 10805  
Confirm with Return.

All images in the brochure – if available – will be displayed.

The background of the screenshot shows search results for 'Picture from 10805', displaying 20 of 27 results. The first result is a VITA VISION 10805 dental crown, with a 'PSD' button next to it. Other results include a VITA VISION 10805 dental crown and a VITA VISION 10805 dental crown.

# Media selection and activities


VITA



Select this asset for download or to add to a collection. Multiple assets can be selected in the gallery.

Direct download of the original file.

Directly add the file to a collection.

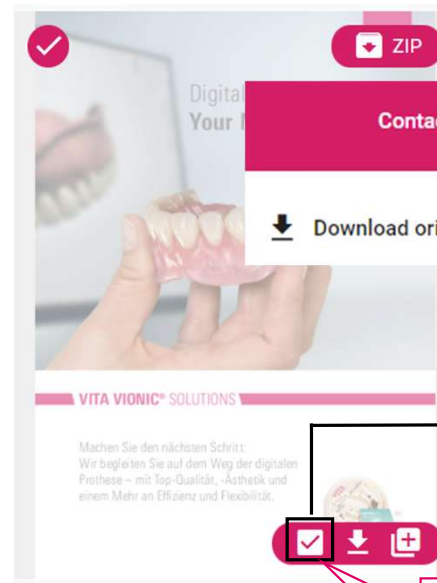

If the "selection checkmark" is set in the window, the options for downloading the (original) file, as well as for adding the original to an collection, appear again in the upper right corner.



# Collection selection

VITA

1

All available collections are displayed here. You can select which collection the file is to be added to.

2

Alternatively, a new collection can be created here, which is then available for collection selection.

The screenshot displays the VITA VIONIC SOLUTIONS app interface. A 'Select collection ...' dialog is open, showing three collections: 'CAD/CAM Material' (36 Elements), 'CAD/CAM Kalender' (5 Elements), and 'Farbbestimmung' (32 Elements). Below the list is a 'Name' input field and a 'Create collection' button. To the right, the 'Add to collection' menu is open, showing options: 'Selection only', 'All results', 'Original', 'Compressed', 'Uncompressed', 'Web', 'Internet', 'Streaming', 'Office', and 'Screen'. A callout box points to the 'All results' option, stating: 'The assets for a specific application can be selected here from all the search results displayed in the gallery. Then loads all assets from the gallery into the collection.'

Select collection ...

- CAD/CAM Material  
36 Elements
- CAD/CAM Kalender  
5 Elements
- Farbbestimmung  
32 Elements

Name

Create collection

+ Add to collection ▾ My collections

Selection only ▸

All results ▸

Original

Compressed

Uncompressed

Web

Internet

Streaming

Office

Screen

The assets for a specific application can be selected here from all the search results displayed in the gallery. Then loads all assets from the gallery into the collection.



# Media information. Detailed view

VITA

The detailed view opens by clicking or double-clicking on the medium – directly below.

Languages and other file formats can be selected in the detailed view for the desired use.

Further information on the medium, such as category, author or print number, can also be viewed.


Linked assets such as images or other PDFs are displayed below the categories by clicking on "Search relatives".

"Search other versions" shows the versions created so far.

The screenshot displays the VITA VIONIC SOLUTIONS media library interface. At the top, there are three thumbnail images of dental models. Below them, the 'VITA VIONIC SOLUTIONS' header is visible. The main content area shows a detailed view of a medium titled 'Digital Dentures: Your Next Level'. To the right of the medium image is a table of 'Media objects' with columns for checkboxes, file names, and formats. Below the table are 'Download' and 'Add to collection' buttons. On the far right, a sidebar contains navigation links for 'Categories' (Products, Removable prosthetics, Digital prosthetics, VITA VIONIC®), 'Types of publication' (Product communication, Brochures), 'Source' (DOTS, Printer Schmerbeck), 'Status' (Free internal+external), 'SAP print number' (10805), 'Owner' (Gatz, Julia), 'Originator' (Layout: DOTS Satz: Druckerei Schmerbeck), and a 'Disclaimer' section. At the bottom of the sidebar are two search buttons: 'Search relatives' and 'Search other versions'.

# Media information. Detailed view

VITA



Digital Dentures:  
Your Next Level

VITA

VITA VIONIC® SOLUTIONS

Machen Sie den nächsten Schritt:  
Wir begleiten Sie auf dem Weg der digitalen  
Prothese – mit Top-Qualität, -Ästhetik und  
einem Mehr an Effizienz und Flexibilität.

### Media objects

<input type="checkbox"/>	10805_VITA-VI...	MA-123...	Original	▼
<input checked="" type="checkbox"/>	10805D_VITA_...	MO-126...	Screen	👁

Name

Number

Languages

Filesize

View PDF

10805D\_VITA\_VIONIC\_SOLUTIONS\_VK  
\_DE\_V02\_screen.pdf

MO-126488

de

2,79 MB

👁

<input type="checkbox"/>	10805E_VITA_...	MO-126...	Screen	👁
<input type="checkbox"/>	10805F_VITA_...	MO-126...	Screen	👁 ▼
<input type="checkbox"/>	10805I_VITA_...	MO-126...	Screen	👁 ▼
<input type="checkbox"/>	10805SP_VITA...	MO-126...	Screen	👁 ▼

Download

Add to collection

Shows the usage. Here is a screen PDF for viewing, not for printing.

The individual file formats are displayed here in the respective languages of the medium.

If the file is a PDF, it can be opened directly in the media database with the Document Viewer via the eye.

The selected file formats can be added to the collection here.



VITA VIONIC SOLUTIONS

🔄 V 002

# My collections

VITA


1



The saved collections can be managed via "My collections".

The number at the top right shows the number of all media objects in all collections. If a media object is added or removed, the number changes accordingly.

2

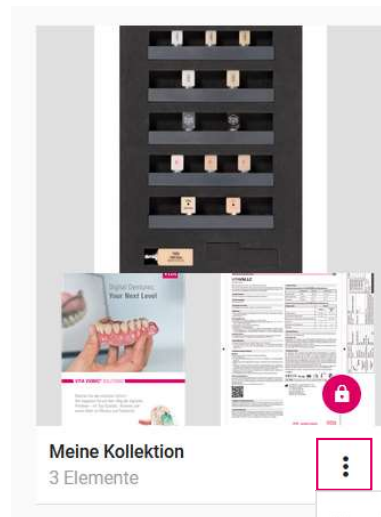


Each user already has a collection available at the beginning. This can neither be renamed nor deleted.

Empty collection

Delete collection

Collections can be emptied or deleted here.

3

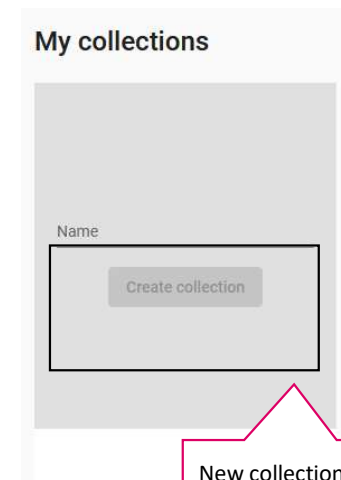

New collections can be created here.

# My collections. Detailed view

VITA

VITA Media database

1

Collections can be renamed using this icon.

2

Clicking on the collection opens it. Here you can download all media objects contained in it, update or share the collection.

Contact & support Change password English Logout

Download all Refresh Share collection

Gallery List Obtainable (5) Approval required (0)

My collections / Test Kollektion

5 Elements

VITA Easyshade® V

ZIP

Original

VITA WiFi-Dongle für VITA Open

ZIP

Original

VITA Easyshade® V

ZIP

Original

VITA Summary of Safety and Clinical Performance

ZIP

Original

VITA ENAMIC® Kurzanleitung

ZIP

Original

3

Individual media objects can also be selected, downloaded or deleted here.

# Postprocessing a collection

VITA


**i Use Case:** only selected media objects from a collection are to be downloaded or deleted.

2


The selected / marked media objects can be downloaded or removed from collection here.


**VITA Media database** [Contact & support](#) [Change password](#) [English](#) [Logout](#)


[Download \(1\)](#) [Remove from collection \(1\)](#) [Download all](#) [Refresh](#) [Share collection](#)


My collections / **Test Kollektion**   
5 Elements


**Gallery** **List** **Obtainable (5)** **Approval required (0)**




**VITA WiFi-Dongle für VITA Öfen**  
Getz auchanweisung  
  
ZIP Original

**VITA Easyshade® V**  
Mod. 4/2016  
  
ZIP Original

**VITA Easyshade® V**  
Quick Start Guide  
  
ZIP Original

**VITA** Summary of Safety and Clinical Performance  
This following SSCP (Summary of Safety and Clinical Performance) is applicable to the following product(s):  
VITA VMAR, VITA VMAR C, VITA VMAR C Prime  
  
ZIP Original

**VITA ENAMIC® Kurzanleitung**  
VITA ENAMIC ist die weltweit einzigartigste Keramik-Vollkronen- und Brücken-Technologie.  
  
ZIP Original


1

The desired media objects can be selected here (multiple selection possible).


You can select whether the media objects are displayed as a gallery in tiles or as a list.

# Share collections

VITA

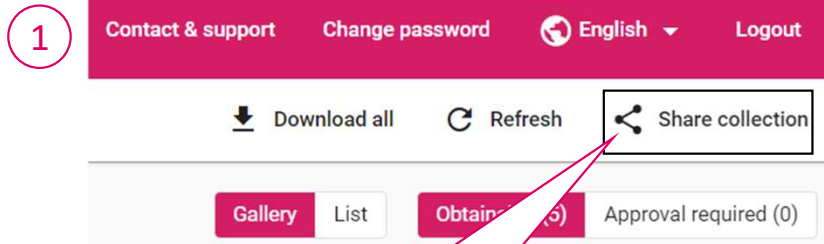

Within a collection, a click on "Share collection" opens the adjacent mask.

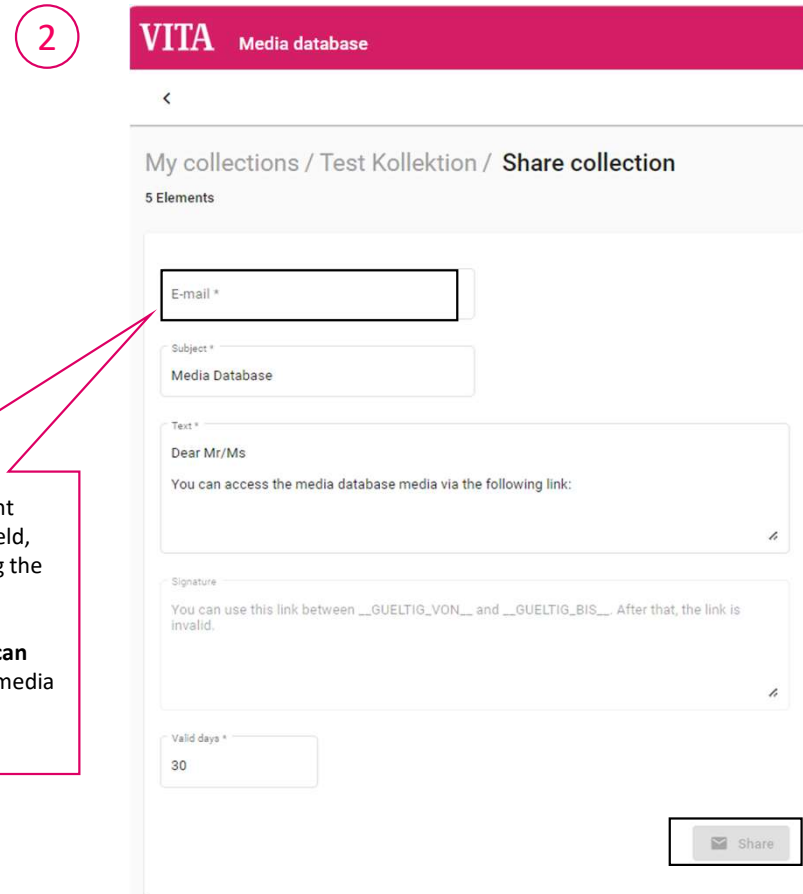

After filling in the desired recipient email address, subject and text field, the collection can be shared using the lower right button "Share".

A link will be sent. **The recipient can open the link** and download the media **without logging in** to the media database.


# Open Document Viewer

VITA




**Attention:** The Document Viewer can only be used for PDF files. Therefore, select the detailed view for brochures that are in ZIP format (as other languages are included). The "eye" symbol appears there for viewing in the Document Viewer.

1

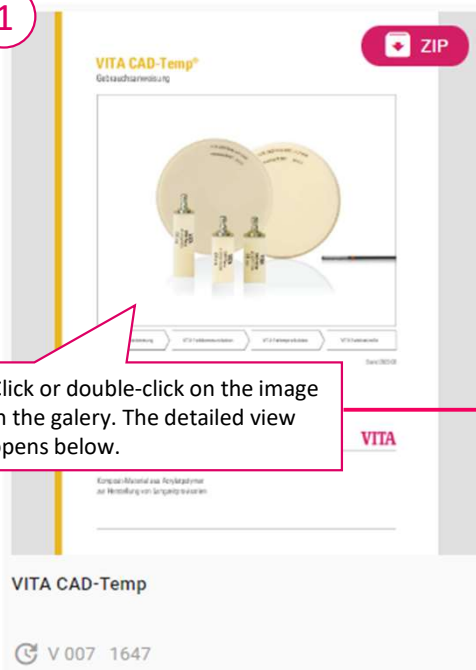

2

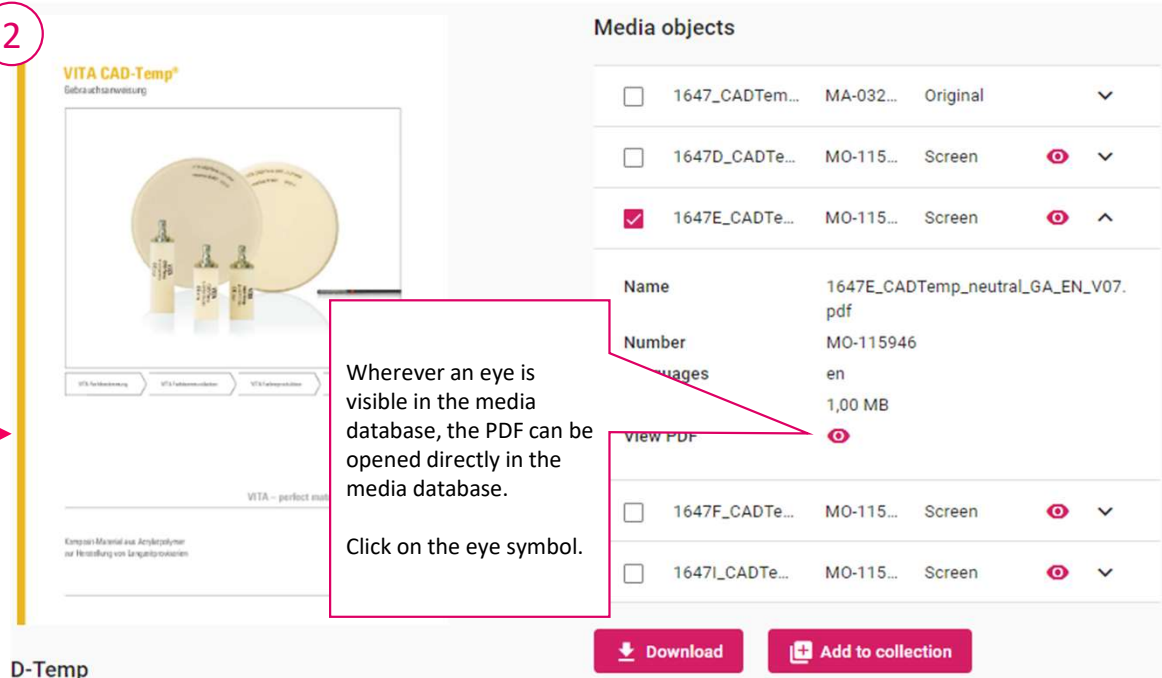





# Document Viewer Properties 1

VITA

**VITA Media database** Contact & support Change password English Logout

112%  

When you click on the page symbol, the thumbnail page view is displayed.

This allows you to change the page view.

This allows text content to be copied directly from the PDF. Mark the desired text.

The magnifying glass can be used to search for terms within the PDF.

**Physical properties**

Properties	Unit
Flexural strength	MPa (N/mm <sup>2</sup> )
Modulus	MPa (N/mm <sup>2</sup> )
Solforming temperature (DSG)	°C
Inorganic filler content	Wt%
Water absorption	complies with EN ISO 10477
Solubility	complies with EN ISO 10477
Shade stability	complies with EN ISO 22172

**Patient target group**  
No restrictions

**Intended user**  
Dental professionals only: dentist and dental technician (fix only).

**Indication and processing requirements**  
VITA CAD-Temp is used for the fabrication of multi-unit, fully or partially anatomical long-term temporary bridge restorations with a span of up to two pontics and a clinical wearing period of up to three years. For CAD/CAM system requirements, please refer to the information provided by the manufacturer of the respective system.

Indication	Anterior crown	Posterior crown	Anterior bridge*	Posterior bridge*
VITA CAD-Temp	●	●	●	●

● recommended \* Only temporary bridges are recommended for wearing periods of more than six months.

**Contraindication**  
Permanent restorations with a clinical wearing period of more than three years. In patients who are allergic to PMMA.

**new shade concept**  
Materials with a single color (monoColor) or four color layers (multiColor) are available.

	0M1T*	1M2T	2M2T	3M2T
CAD-Temp monoColor				
CAD-Temp multiColor				

\* For the reproduction of bleached teeth (only available in size C1-40)

**Preparation guidelines**  
Since VITA CAD-Temp restorations normally provide the basis for definitive all ceramic restorations, the standard guidelines for the preparation of all ceramic restorations must be observed. For detailed information, see the brochure "Clinical Aspects of All Ceramics, new, revised".

**Benefits**

- The material is suitable for restorations with a clinical wearing period of up to three years.\*
- Homogeneous material due to innovative manufacturing process
- Well balanced combination of mechanical properties such as tensile strength and elasticity, for clinical use and the specific indication.
- Excellent abrasion resistance (see literature).
- Translucency and fluorescence based on natural dentition.
- Radiopaque
- Good polishing characteristics.
- Can be individualized with the light curing VITA VM LC and VITA VM LC flow microparticle composite.
- Can be characterized with shades using VITA AKZENT LC

**Functions of temporary restorations made from VITA CAD-Temp**

- Prophylactic functions:**
  - avoiding the movement of abutment teeth
  - protecting the tooth substance against bacterial, toxic and thermal effects
- Diagnostic and esthetic functions:**
  - checking occlusion
  - checking phonetics
  - checking the vertical dimension
  - checking the esthetic result
- Therapeutic functions:**
  - gingival forming for controlled papillary growth for later implementation in all ceramic restorations
  - restoring implants during the healing phase
  - correction of temporomandibular joint disorders
  - correction of the occlusal plane

# Document Viewer Properties 2

VITA

**VITA Media database** Contact & support Change password English Logout

112% [-] [+] [Hand] [Reset]

**Page Transition**

- Continuous Page
- Page by Page

**Page Orientation**

- Rotate Clockwise
- Rotate Counterclockwise

**Page Layout**

- Single Page
- Double Page
- Cover Facing Page

**Physical properties**

Properties	Unit	Value*
Flexural strength	MPa (N/mm <sup>2</sup> )	>80
Modulus	MPa (N/mm <sup>2</sup> )	approx. 2800
Solubility temperature (DSC)	°C	approx. 110
Inorganic filler content	Wt%	approx. 14
Water absorption	complies with EN ISO 10477 Polymer based crown and bridge materials	
Solubility	complies with EN ISO 10477 Polymer based crown and bridge materials	
Shade stability	complies with EN ISO 27117 Artificial teeth for dental prostheses	

\* The technical/physical values are typical measuring results and refer to internal samples and measurement equipment available on site. If samples are prepared using different methods and measurement equipment, other measuring results may be produced.

**Patient target group**  
No restrictions

**Intended user**  
Dental professionals only: dentist and dental technician (Rx only).

**Indication and processing requirements**  
VITA CAD Temp is used for the fabrication of multi unit, fully or partially anatomical long term temporary bridge restorations with a span of up to two pontics and a clinical wearing period of up to three years. For CAD/CAM system requirements, please refer to the information provided by the manufacturer of the respective system.

Indication	Anterior crown	Posterior crown	Anterior bridge*	Posterior bridge*
VITA CAD Temp	●	●	●	●

● recommended \* Only temporary bridges are recommended for wearing periods of more than six months.

**Contraindication**  
Permanent restorations with a clinical wearing period of more than three years. In patients who are allergic to PMMA.

**The shade concept**  
Materials with a single color (monoColor) or four color layers (multiColor) are available.

	0M1T*	1M2T	2M2T	3M2T
CAD-Temp monoColor				
CAD-Temp multiColor		1M2T	2M2T	3M2T

\* For the reproduction of bleached teeth only available in size C1-40

**Preparation guidelines**  
Since VITA CAD Temp restorations normally provide the basis for definitive all ceramic restorations, the standard guidelines for the preparation of all ceramic restorations must be observed. For detailed information, see the brochure "Clinical Aspects of All Ceramics" No. 1696

**Benefits**

- The material is suitable for restorations with a clinical wearing period of up to three years.\*
- Homogeneous material due to industrial manufacturing process
- Well balanced combination of mechanical properties, such as tensile strength and elasticity, for clinical use and the specific indication.
- Excellent abrasion resistance (see literature).
- Translucency and fluorescence based on natural dentition.
- Radioopaque
- Good polishing characteristics.
- Can be individualized with the light curing VITA VM LC and VITA VM LC flow microparticle composite.
- Can be characterized with shades using VITA AK/ZENT LC

**Functions of temporary restorations made from VITA CAD-Temp**

- Prophylactic functions:**
  - avoiding the movement of abutment teeth
  - protecting the tooth substance against bacterial, toxic and thermal effects
- Diagnostic and esthetic functions:**
  - checking occlusion
  - checking phonetics
  - checking the vertical dimension
  - checking the esthetic result
- Therapeutic functions:**
  - gingival forming for controlled papillary growth for later implementation in all ceramic restorations
  - restoring implants during the healing phase
  - correction of temporomandibular joint disorders
  - correction of the occlusal plane

Search document Full screen Download Print Dark mode Language

3


This opens the Page view menu.

Dragging the area for the thumbnail side view.

A download can also be started here by clicking on the Settings icon.

# Request release of images 1


VITA

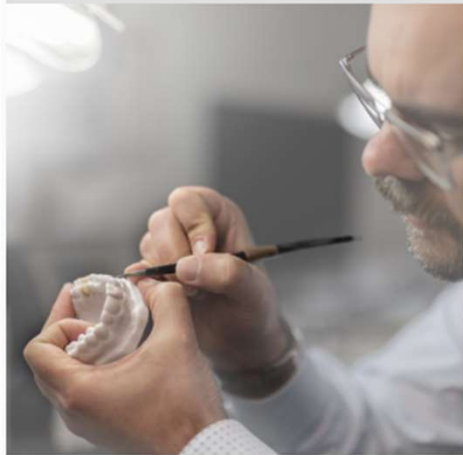

JPG

VITA LUMEX AC. P. Schäfer layers a crown

Application pictures V 007 10605



JPG

VITA LUMEX AC. Powerwash

Application pictures V 007 10605

VITA LUMEX AC. P. Schäfer layers a crown

Image from 10605 V07 Crown. Layering. 0254 Alexandra Weiss Publication only to VITA customers with attribution: © Alexandra Weiss

V 007

10605

MA-130049

Created on  
31/07/2024

Categories

Products ▶ Veneering ▶ All-ceramics ▶ VITA LUMEX® AC

Media by Categories ▶ Products ▶ Application pictures

Source ▶ Alexandra Weiss

Status

Free internal+external for inquiry

The status “Free internal+external for inquiry” indicates that this image or document is locked. A release request is necessary.

# Request release of images 2

VITA




VITA LUMEX AC. P. Schäfer layers a crown

Application pictures V 007 10605




VITA LUMEX AC. Powerwash

Application pictures V 007 10605

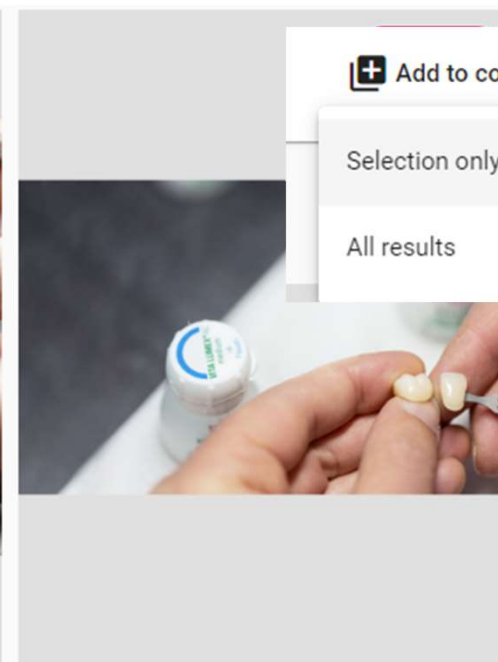

VITA LUMEX AC. Shade matching

Application pictures V 007 10605

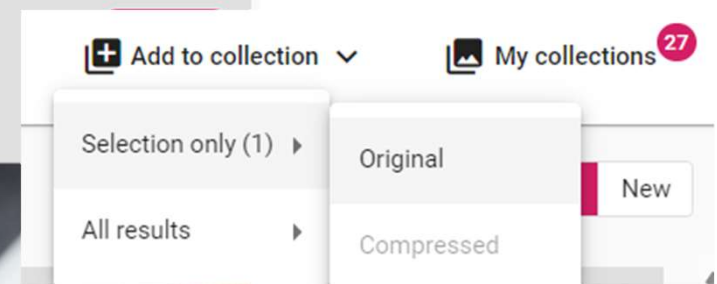

1. select images
2. add to collection
3. switch to "My collections"

# Request release of images 3

VITA

VITA



My collections / Release of LUMEX AC 

5 Elements

Gallery

List

Obtainable (5)

Approval required (2)

1

Switch between “Obtainable” and “Approval required” to see the images for which approval is required.

 PNG

Internet

2

Select the images in the “Approval required” tab. **Check the box next to each picture.**





# Request release of images 4

VITA

< Remove from collection (2) Submit approval request (2) Refresh

My collections / Release of LUMEX AC ✎

2 Elements

Gallery List Obsolete (5) Approval required (2)

1

Once all images have been selected, click on **"Submit approval request"**.

2

This message will then appear at the bottom right of the browser.

An approval request for 1 element has been submitted.

# Request release of images 5

VITA



- The release is processed by VITA.
- You will receive an e-mail when the media has been released.

After receiving the release e-mail, the media can now be downloaded under **“Obtainable”**.



Download all Refresh Share collection

My collections / Release of LUMEX AC

6 Elements

Gallery List Obtainable (6) Approval required (1)

JPG



Original

PNG



Internet

PNG



Internet

PNG



Internet

PNG



Internet



# Contact

# VITA

## Media requests and contact

VITA Zahnfabrik

H. Rauter GmbH & Co. KG

Ina Bretschneider

E-Mail: [i.bretschneider@vita-zahnfabrik.com](mailto:i.bretschneider@vita-zahnfabrik.com)

T: +49 (0) 7761 / 562-502

## Technical support

it.x informationssysteme gmbh

Customer Support

E-Mail: [support@itx.de](mailto:support@itx.de)

T: +49 (0) 75 31 / 89 27 300

F: +49 (0) 75 31 / 89 27 329

**VITA Zahnfabrik H. Rauter GmbH & Co. KG**

Spitalgasse 3

D-79713 Bad Säckingen

Germany



<https://vita-zahnfabrik.com>



FACEBOOK Follow us



INSTAGRAM Follow us